



中国认可
国际互认
检测
TESTING
CNAS L9334



微谱
WEIPU

Test Report

Report No. : WP-21126225-JC-02EnR1

SampleOrigin : Customer Sample Delivery

Client : GRIS CUBRICA

Address: /

Shanghai WEIPU Chemical Technology Service Co., Ltd



Report No. : WP-21126225-JC-02EnR1 Page(s) : 1 / 4

Test Report

The following sample(s) was/were submitted and identified on behalf of the applicant:

Sample Name: Please refer to next page(s).

Sample character: Solid

Type: /

Testing information:

Date of Sample Received: 2021-12-13

Testing Period: 2021-12-13~2022-01-06

Test Item(s): Selected test (s) as requested by client.

Test Criterion: Please refer to next page(s).

Test Result: Please refer to next page(s).

Complied by :

Daryimin

Approved by :

Caina Min

Issued Date :

2022-01-12



Report No. : WP-21126225-JC-02EnR1 Page(s) : 2 / 4

Sample information

Sample ID	Sample Name
211203834-1	Product in same trade
211203834-2	Gris cubrica

1. Test Item : Ultraviolet aging

Test Method: GB/T 14522-2008

Test Equipment:

Ultraviolet aging tester, Model: QUV/Spray

Test condition(s):

Ultraviolet aging Test condition(s):


UVA-340 light source, irradiance: 0.76 W/ (m²•nm) , exposure to radiation at black-panel temperature 60 °C for 8h; no radiation condensation exposure for 4 h at black-panel temperature of 50 °C.

Total test time: 500 h

Test result(s)


Sample ID	Sample Description	Test Items	Test results
211203834-1	/	Ultraviolet aging	Slight change in visual color (slight blueness, speckled appearance)
211203834-2	/		No change in visual color

Representative attachments:

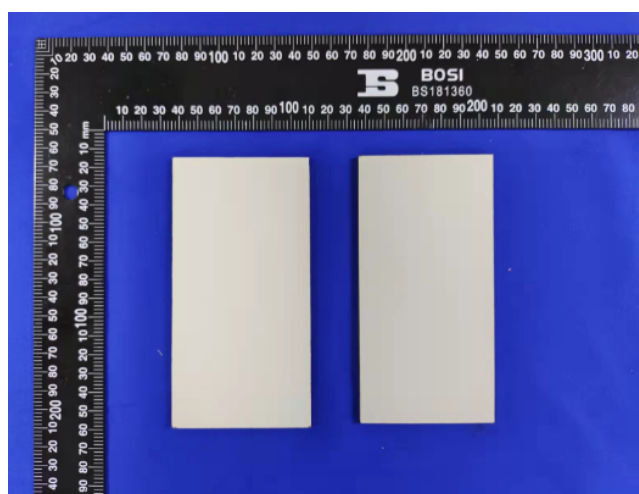

Before test(left: 211203834-1, right: 211203834-2)


Report No. : WP-21126225-JC-02EnR1 Page(s) : 3 / 4

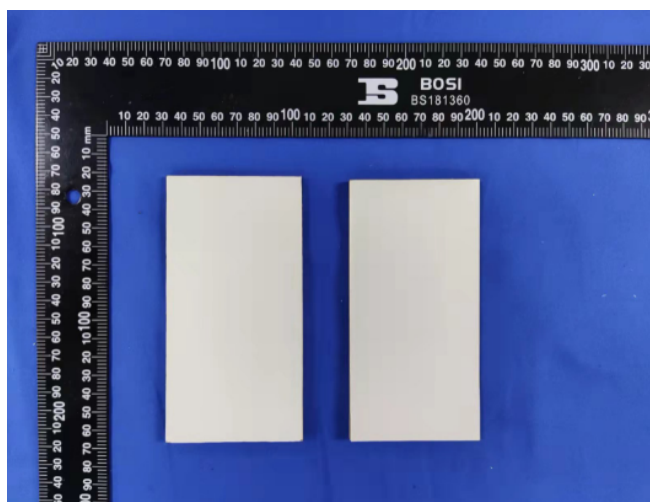

After test (left: 211203834-1, right: 211203834-2)



211203834-1 Color change

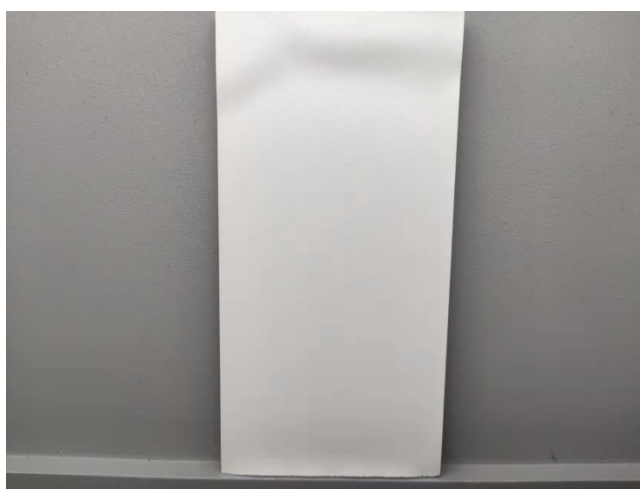

211203834-2 Color change

Report No. : WP-21126225-JC-02EnR1 Page(s) : 4 / 4

Note: This Report cancels and supersedes the Report No·WP-21126225-JC-02En issued by Micro spectrum Technology Co., Ltd,
original report will be invalid from today.

End of the Report

——DECLARE——

1. The report is invalid without the stamp of“Special Seal for Inspection or Testing” or without“Special Seal for the Report” or without the signature of the compiler and the approver.
2. No unauthorized changes, additions or deletions shall be made to the report.
3. Neither fragmented report nor its incomplete copy shall be deemed valid. The complete copy is invalid without the stamp of“Special Seal for Inspection or Testing” or “Special Seal for the Report”.
4. Any queries on the report shall be presented to us within 15 working days after receipt of the report.
5. The results described here in this report are based on the sample(s) tested.The data and results shown in the report without CMA logo are not used as proof for society, only for internal uses.
6. The applicant takes full responsible for the truthfulness of the testing sample(s) and information related thereto.
7. Without the permission of the company, any party is prohibited from using the test results and the report for undue publicity.

